

HIV Testing Technology and the Latest Algorithm

David Warshauer, PhD, D(ABMM)


Deputy Director, Communicable Diseases

Wisconsin State Laboratory of Hygiene






HIV Testing has changed over time

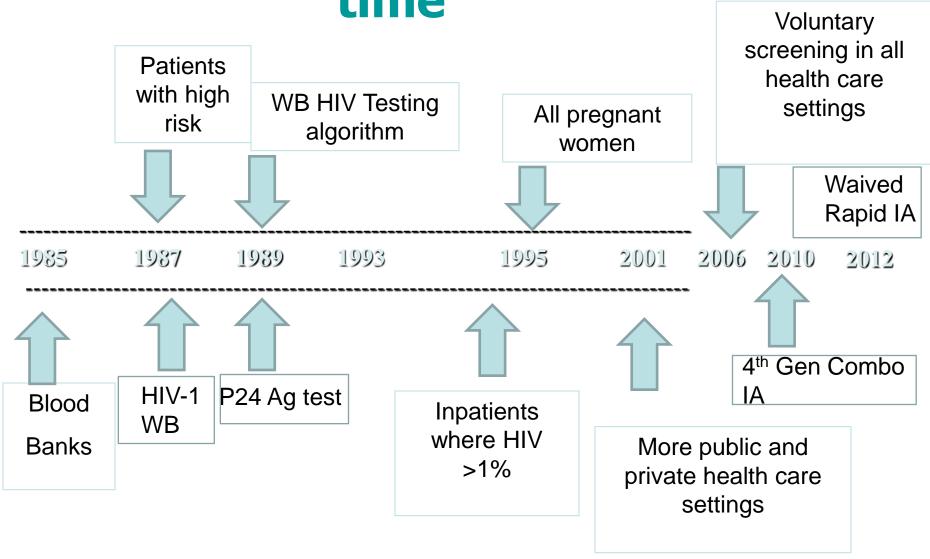





1989 HIV Algorithm

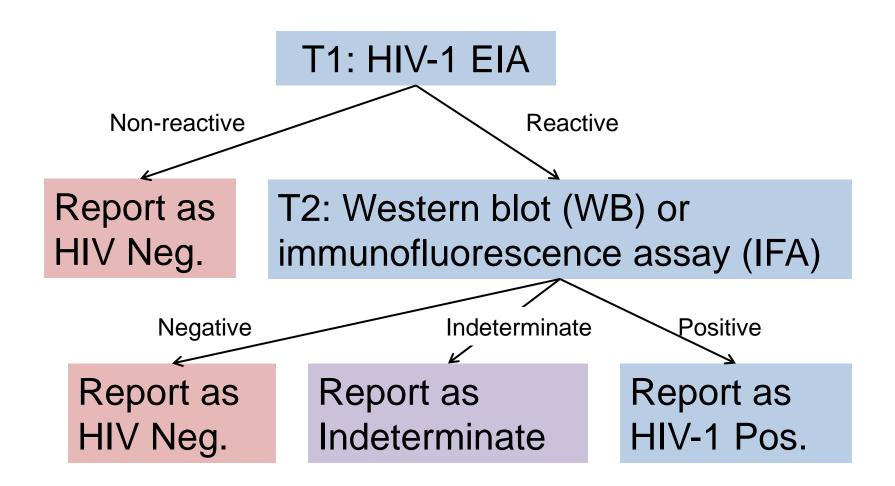






New HIV testing strategies/algorithms

- 1989 algorithm remained largely unchanged for over 30 years
- Learned more about HIV-1 and HIV-2 disease
 - Disease progression
 - Virus dynamics
 - Window Period
- Advancements in technology and molecular tests





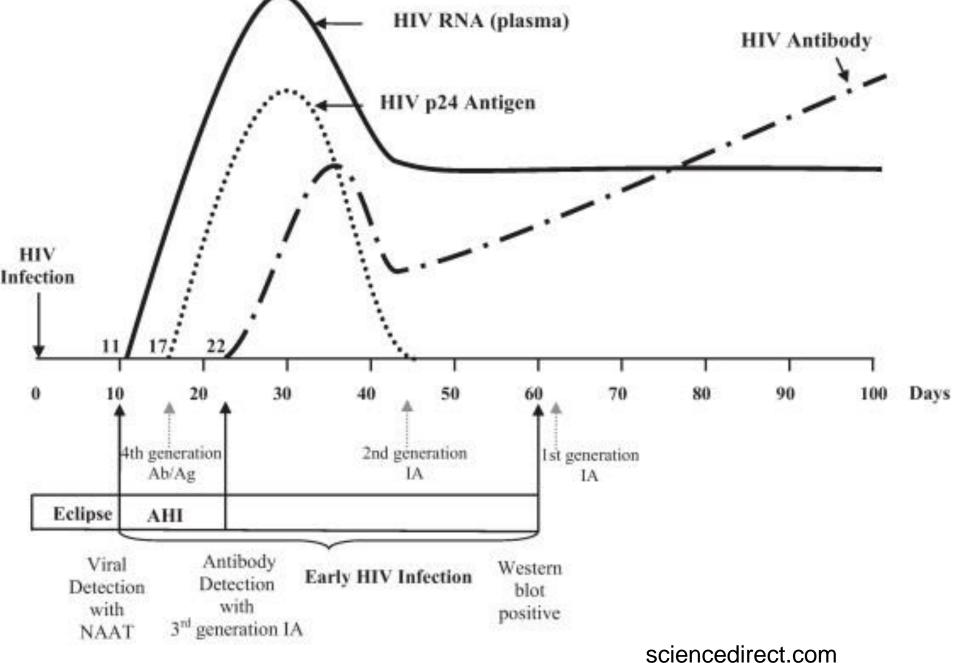

Evolution of the HIV Immunoassays

- Designed for sensitivity and use as screening tests
- Reactive result considered "preliminary positive"
 - Supplemental testing needed to confirm
- IAs have become more sensitive with each new generation
 - 1st gen EIA: HIV-1 viral lysates; indirect IA using labeled antihuman IgG
 - Required significant dilution to overcome non-specific reactions with cellular protein contaminants





Evolution of the HIV Immunoassays

- 1991---2nd gen IA: Improved sens & spec
 - HIV-1/HIV-2
 - Synthetic peptide or recomb Ag w/wo viral lysates
 - IgG
- 1992---3rd gen IA: HIV-1/HIV-2
 - synthetic peptide or recomb Ag
 - IgM + IgG Ab
 - Ag sandwich format; lower specimen dilution; increased sensitivity



Evolution of the HIV Immunoassays

- 2010---4th gen IA
 - Similar to 3rd gen w/ addition of p24 Ag detection
- 5th gen multiplex flow IA:
 - differentiates HIV-1 Ag, HIV-1 and HIV-2
 Ab (Bio-Rad)

4th Generation HIV Ag/Ab Combo Assays

Test Name (Manufacturer)	Instrument	Specimen Types	Result Output
Abbott ARCHITECT HIV Ag/Ab Combo (Abbott Diagnostics)	Fully automated, random access (i2000SR)	Serum Plasma	Nonreactive Reactive
GS HIV Combo Ag/Ab EIA (Bio-Rad Laboratories)	Manual or semi- automated instrument (Evolis)	Serum Plasma	Nonreactive Reactive
ADVIA Centaur HIV Ag/Ab Combo (Siemens Healthcare Diag.)	Fully automated, random access (Centaur/Centaur XP)	Serum	Nonreactive Reactive





4th Generation Ag/Ab Test

- 3 FDA-approved kits available
 - ARCHITECT HIV Ag/Ab Combo (Abbott)
 - GS HIV Ag/Ab Combo EIA (Bio-Rad)
 - ADVIA Centaur Ag/Ab CIA
- Detect HIV-1 p24 Ag, HIV-1 and HIV-2 antibodies
- Reactive result:
 - Doesn't distinguish between Ag and Ab
 - Preliminary positive
 - Supplemental testing required





5th Generation Ag/Ab Test

- BioPlex 2200 HIV Ag/Ab Test
 - Detects and differentiates HIV-1 Ag, HIV-1 Ab, and HIV-2 Ab in serum or plasma
 - Early infection detection similar to other laboratory Ag/Ab tests
 - High sensitivity and specificity
 - Further data needed on performance in the algorithm





Changes that impact HIV testing strategies/algorithms

- Evolving technology
 - Availability of rapid tests
 - Increased sensitivity of screening assays
 - Western blot and IFA now much less sensitive than screening assays which they are intended to "confirm"






Western blot (WB)

- Designed for specificity
- Must meet specific criteria for a positive interpretation
- Indeterminate results occur for a variety of reasons
 - Early infection, late infection, HIV-2 infection, other
- Western blot technology has not advanced
 - Newer immunoassays are more sensitive than WB
- Lack of sensitivity can lead to false negative and inconclusive results





Sequence of HIV Assay Reactivity During Early HIV Infection Relative to Western Blot*

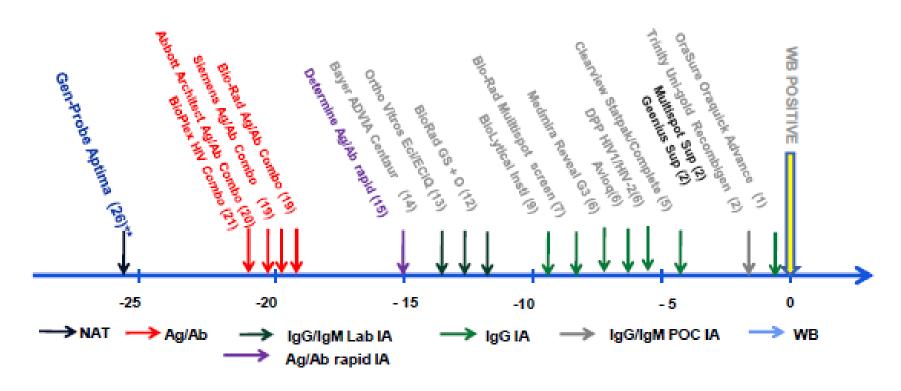

^{*}Assay sensitivity above is based on frozen plasma only. Whole-blood and oral fluid has not been characterized for early infection.
**Current data suggests that the Gen-Probe Aptima can detect HIV-1 RNA ~5-28 days after infection.

Adapted from Owen et al J Clin Micro 2008 and Masclotra et al J Clin Virol 2011





HIV Test Strategy Workgroups

- Two workgroups were formed in October 2006
 - Focused on strategies for both POC and Laboratory settings
- HIV Diagnostics Conference in December 2007
 - Data was presented to substantiate various algorithms
- Status Report started fall 2008
 - APHL/CDC Steering Committee produced a report of the current status of the proposed algorithms





- 2010 HIV Diagnostics Conf.
 - Announced consideration of Multispot as suppleImental assay
- 2012 HIV Diagnostics Conf.
 - Draft recommendations for a new HIV testing algorithm
- 2014 HIV Diagnostics Conf.
 - CDC publishes new HIV testing algorithm





Representation on Laboratory and POC Workgroups

- Association of Public Health Laboratories
- American Clinical Laboratory Association
- American Society of Microbiology
- Blood Banks
- College of American Pathologists

- US Centers for Disease Control and Prevention
- Commercial Laboratories
- US Department of Defense
- US Food and Drug Administration
- HIV Program Staff from NASTAD and Public health departments





What are we looking for from these new testing strategies?

- Resolution of indeterminates
- Ability to confirm HIV-2 infections
- Increased detection of acute infection
- Assays that can be used as screening or confirmatory/ supplemental tests and as part of multitest algorithms
- Guidance for laboratory confirmation of POC rapid tests







Laboratory Algorithms








New CDC Recommendations for HIV Testing in Laboratories

A step-by-step account of the approach

CDC's new recommendations for HIV testing in laboratories capitalize on the latest available technologies to help diagnose HIV infections earlier – as much as 3-4 weeks sooner than the previous testing approach. Early diagnosis is critical since many new infections are transmitted by people in the earliest ("acute") stage of infection.

By putting the latest testing technology to work in laboratories across the United States, we can help address a critical gap in the nation's HIV prevention efforts.

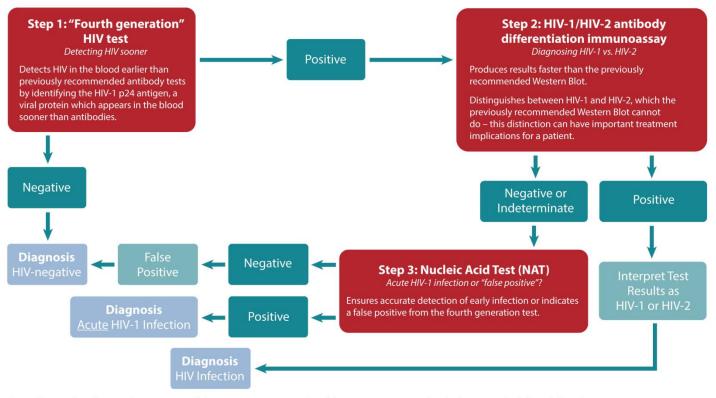

This graphic is designed to illustrate key concepts of the new testing approach in laboratories. For more detail, please see the full guidelines here: http://www.cdc.gov/hiv/pdf/HIVtestingAlgorithmRecommendation-Final.pdf.



U.S. Department of Health and Human Services

Centers for Disease Control and Prevention


www.cdc.gov/nchhstp/newsroom

JUNE 2014





Algorithm with 5th Generation Test

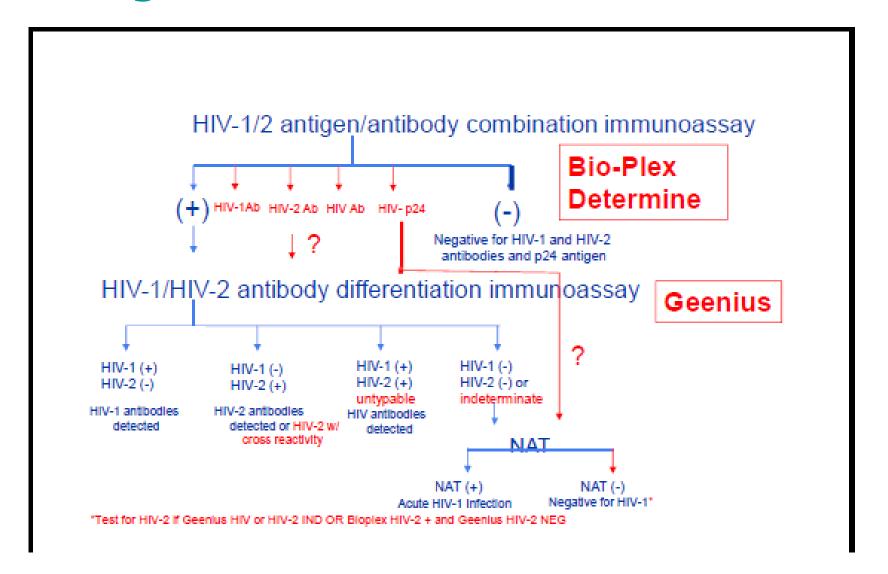





Advantages of the New Algorithm

- 4th Gen Ag/Ab more sensitive and specific
- Allows detection of acute HIV infection
- Eliminates expensive, labor intensive, and problematic WB
- Allows detection of HIV-2 infection
- Geenius HIV-1/HIV-2 is simple, rapid, and less expensive than WB





HIV-1 NAT

- Only one HIV-1 RNA test FDA-approved for use as an aid in the diagnosis of HIV-1 infection
 - APTIMA® HIV-1 RNA Qualitative Assay (Gen-Probe)
- Several HIV-1 quantitative tests (viral load)
 - FDA approval is for patient monitoring, i.e. assess prognosis, monitor effects of therapy
 - Not intended as a diagnostic test to confirm the presence of HIV-1 infection
- WSLH using proviral DNA RT-PCR





HIV-1/HIV-2 Discriminatory Immunoassay

Multispot HIV-1/HIV-2 Rapid Test


FDA-approxed:

To detect & <u>differentiate</u> antibodies

Suitable for multi-test algorithms

 Current package insert does not sp supplemental test






Results in 30 min

Not CLIA waived

Seram or plasma



HIV-1 recombinant

HIV-1 peptide

HIV-2 peptide



Geenius HIV 1/2 Supplemental Assay





Geenius HIV 1/2 Supplemental Assay

- FDA approved Oct 2014
- Replaces Multispot
- Differentiates HIV-1 and HIV-2 antibodies
- 30 minutes



Geenius



Protein A colloidal gold detection

Test Antigens (lines, left to right)

- 1. HIV-2 gp36 (env peptide)
- HIV-2 gp140*
- 3. HIV-1 p31 (pol peptide)
- HIV-1 gp160 (env recomb prot)
- HIV-1 p24 (core recomb prot)
- HIV-1 gp41(env peptides)
- Control (protein A)

^{*}Multimer of HIV-2 gp36 env peptide

Geenius™ Compared to Multispot

Multispot	Geenius
Rapid testing (2004) or Supplemental (2013)	Supplemental use only (confirmation)
Manual reading and interpretation	Geenius Reader and automatic interpretation on Geenius Software
Manual result entry into LIS/LIMS	Bi-directional connection to LIS/LIMS
Manual labeling	Full traceability; barcode identification
Dilution protocol in PI to resolve cross- reactivity	No Equivalent
Serum or plasma	Serum, plasma, fingerstick or venous whole blood





Geenius™ and Multispot Results

Multispot Results	Geenius Results	
Nonreactive	Nonreactive	
Reactive: HIV-1 positive	Reactive: HIV-1 positive	
Reactive: HIV-2 positive	Reactive: HIV-2 positive	
No Equivalent	Reactive: HIV-2 positive with HIV-1 cross-reactivity	
Reactive: HIV positive (undifferentiated)	Reactive: HIV positive untypable (undifferentiated)	
Indeterminate: HIV-1 indeterminate	Indeterminate: HIV-1 indeterminate	
No Equivalent	Indeterminate: HIV-2 indeterminate	
No Equivalent	Indeterminate: HIV indeterminate	





- HIV-2 positive with HIV-1 cross-reactivity
 - Antibody to HIV-2 confirmed
 - HIV-1 reactivity does not meet criteria to be considered positive
 - only one HIV-1 envelope band detected
 - Gp160 or gp41
 - Indicative of HIV-1 cross-reactivity
 - Final Interpretation Reported
 - HIV-2 Positive
 - Patient should be referred to care for HIV-2 infection





What results are seen with HIV-2 Ab positive specimens?

- Package Insert Data for 200 specimens
 - HIV-2 Positive for 38.5% (77/200)
 - HIV-2 with HIV-1 cross-reactivity for 54% (108/200)
 - HIV Undifferentiated for 6% (12/200)
 - HIV indeterminate for 1.5% (3/200)



HIV-2 Indeterminate

- Repeat before reporting
- If repeat is "HIV-negative, report as such
- If repeat is "HIV-1positive" or HIV-2 positive", report as such
- If repeat is HIV-2 indeterminate, report as HIV-2 indeterminate
 - Result may indicate acute HIV-1 infection
 - HIV-1 NAT should be performed





- HIV-2 Indeterminate (con't)
 - If HIV-1 NAT is negative
 - Refer specimen for testing with a different HIV-2 test
 - Or repeat testing in 2-4 weeks



HIV Indeterminate

- Bands present for both HIV-1 and HIV-2,
 but positive criteria not met for either
- Repeat before reporting
- If repeat is "HIV-negative, report as such
- If repeat is "HIV-1positive" or HIV-2 positive", report as such
- If repeat is HIV indeterminate, report as HIV indeterminate
 - Result may indicate acute HIV-1 infection
 - HIV-1 NAT should be performed





- HIV indeterminate
 - Perform HIV-1 NAT
 - If NAT pos, refer patient to care for HIV-1
 - If NAT neg, refer specimen for HIV-2 testing with NAT or different antibody test
 - or repeat testing in 2-4 weeks

- HIV-1 indeterminate
 - Same testing sequence as for HIV indeterminate with except additional HIV-2 testing is not necessary



Geenius Results-What They Mean


- HIV Positive Untypable (undifferentiated)
 - Antibodies to HIV-1 and HIV-2 confirmed in the specimen
 - May occur in an HIV-2 positive sample with significant cross-reactivity to HIV-1
 - Or co-infection with both HIV-1 and HIV-2
 - Repeat to confirm before reporting
 - Interpret similar manner as "HIV indeterminate"



Geenius Results-What They Mean

- HIV Positive Untypable (undifferentiated)
 - Perform HIV-1 NAT
 - If NAT pos, refer patient to care for HIV-1
 - If NAT neg, refer specimen for HIV-2 testing with NAT or different antibody test

repeat testing in 2-4 weeks









Geenius Results Reporting

Not
Reported

		Reported
HIV-l result	HIV-2 result	G eenius Assay Interpretation
Negative	Negative	H I V Negative
Indeterminate	Negative	HIV-l Indeterm in a te
Negative	Indeterminate	HIV-2 Indeterminate
Indeterminate	Indeterminate	HIV Indeterminate
Positive	Negative	HIV-1 Positive
Positive	Indeterminate	HIV-1 Positive
Negative	Positive	HIV-2 Positive
Indeterminate	Positive	HIV-2 Positive
Positive	Positive	HIV-2 POSITIVE with HIV-1 cross-reactivity: Antibody to
		HIV-2 confirmed in the sample. HIV-1 positivity (with only one HIV-1 envelope band, gp160 or gp41), is due to cross-reactivity and
		precludes confirmation of HIV - 1.*
		*Note: Differentiation features managed by proprietary algorithm.
Positive	Positive	HIV POSITIVE Untypable (undifferentiated): Antibodies to
		HIV-1 and HIV-2 confirmed in the sample. This may occur in an
		HIV-2 positive sample with significant cross-reactivity to HIV-1, or
		may be due to co-infection with both HIV -1 and HIV -2 (rare).*
		*Note: Differentiation features managed by proprietary algorithm










Approved Tests for the Point of Care



Uni-Gold Recombigen






OraQuick ADVANCE



Clearview Complete HIV 1/2

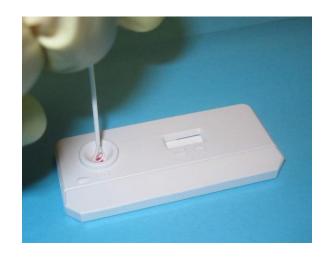

Clearview HIV 1/2 Stat Pak



Reveal

G3

Product	Specimen type	CLIA Category	Exp.
Unigold	Whole Blood	Waived	1 yr
Recombigen HIV	Serum, Plasma	Moderate Complexity	
OraQuick	Oral Fluid, Whole Bld	Waived	6
ADVANCE HIV 1/2	Plasma	Moderate Complexity	mos.
Reveal G3 Rapid HIV-1	Serum, Plasma	Moderate Complexity	1 yr
Clearview	Whole Blood	Waived	2 yrs
STAT-PAK HIV-1/2	Serum, Plasma	Moderate Complexity	
Clearview	Whole Blood	Waived	2 yrs
Complete HIV-1/2	Serum, Plasma	Moderate Complexity	
Alere Determine	Whole Blood	Waived Moderate Complexity	15 mo





FDA Approved HIV Rapid Tests

Product	Manufacturer	Analyte	Specimen Type	Sensitivity	Specificity	FDA Approval
Unigold Recombigen HIV	Trinity Biotech www.trinityusa.com	HIV-1	Whole blood, Serum, Plasma	100%	99.7%	Dec. 2003
OraQuick ADVANCE HIV 1/2	Orasure Technologies www.orasure.com	HIV-1 HIV-2	Whole blood, Oral fluid, Plasma	99.6% BL 99.3% OF	100% BL 99.8% OF 99.9% plasma	June 2004
Reveal G3 Rapid HIV-1	MedMira www.reveal-hiv.com	HIV-1	Serum, Plasma	99.8%	99.1% serum 98.6% plasma	Oct. 2006
Clearview STAT-PAK HIV-1/2 & Complete HIV-1/2	Inverness Med. www.invernessmedical pd.com	HIV-1 HIV-2	Whole blood, Serum, Plasma	99.7%	99.9%	May 2006
Determine HIV-1/2 Ag/Ab	Alere www.alerehiv.com	HIV-1 Ab HIV-2 Ab HiV-1 Ag	Whole blood, serum, plasma	99.9	99.7% BL 99.6% serum 99.7% plasma	2013,2014





Non-Clinical Site Algorithms


- Single rapid test with immediate linkage to clinical provider if reactive
- Single rapid test followed by lab-based follow up testing if reactive
 - WDPH algorithm for CTS
- Single rapid test immediately followed up a 2nd rapid test on-site if reactive
 - If both tests reactive, link to HIV care
 - If second test nonreactive, refer to laboratory or clinical provider for follow-up testing





Testing Strategy for Point of Care HIV Rapid Testing Facilities

Two Rapid Tests (A1/A2) Performed in Sequence on Blood (A1 and A2 must be different rapid tests)

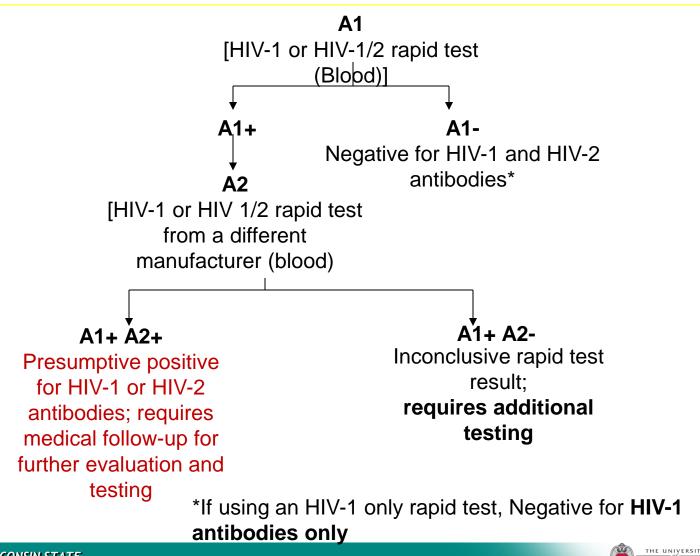

POC Two Test Algorithm

- Requires that technicians be proficient with 2 tests
 - Limited training, expertise required
- Little chance for false-positive or false-negative algorithm results
- Likely to work well in high prevalence settings
- In low prevalence areas majority of specimens will require lab resolution





POC Testing using Multi-Rapid Test Algorithms

- Addresses low return rate for confirmatory test results experienced in some settings
- Can optimize care and treatment for HIVinfected persons
 - HC settings can aid in definitive diagnosis and therefore inform clinical decisions quickly
 - All settings can facilitate referral to HIV care, especially with mobile and transient populations
- Can optimize prevention
 - Messages about HIV test results can be clearer and more persuasive; optimizes prevention and care engagement
 - Facilitates provision of partner services





Oral Fluid Testing

- Not part of CDC's recommended algorithm
- Requires a testing algorithm that includes the Western blot
- Does not detect infection as early as blood tests



More Information

 CDC and APHL. Laboratory testing for the diagnosis of HIV infection: updated recommendations. http://stacks.cdc.gov/view/cdc/23447

- APHL.HIV Diagnostic Informational Updates Modified on March 17, 2016. https://www.aphl.org/programs/infectious_disease/ Documents/2015_Informational%20Update_02_12 16_FINAL.pdf
- Link to 2016 HIV Diagnostic Conference: http://hivtestingconference.org/



